

OHD Fit Test Adapter | Kit #20

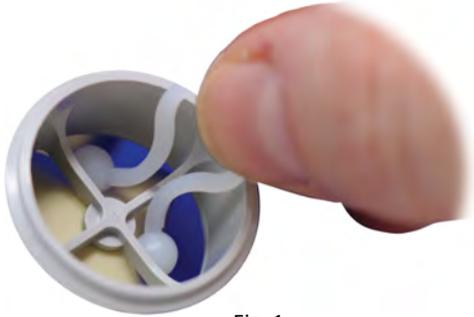


Fig. 1



Fig. 2

INSTRUCTIONS:

1. Prop open or remove the inhalation valve on the front of the mask (Fig. 1 – valve will not match image exactly)
2. Insert the adapter in the front of the mask like you would install a cartridge
3. Connect the clear tubes to the two-connector part and the blue tube to the single-connector part (Fig. 2)
4. Perform fit test

CARE:

1. The adapters should be handled with care so as not to create damage that might interfere with testing.
2. Periodically check the metal hose connectors to be sure they are secure.
3. If the diaphragm should leak on the single-port side of the adapter, remove 8 screws on top, carefully line up new diaphragm, screw in the screws loosely. Tighten opposite sides until all are secure.
4. Adapters may be cleaned with soapy water and soft cloth.
5. Adapters can be disinfected by spraying a disinfectant between tests or immersed in a cleaning solution and left out to dry. (The adapters allow outside air to be inhaled, but an employee's exhalation is routed through the exhalation valve nullifying the risk of cross-contamination.)



Fit Test Adapter Kit #20 For Sundstrom

